

FIG. 1

## ${\it SYSTEM~AND~METHODS~FOR~PROCESSING~ANALYTE~SENSOR}$

DATA Goode, et al.

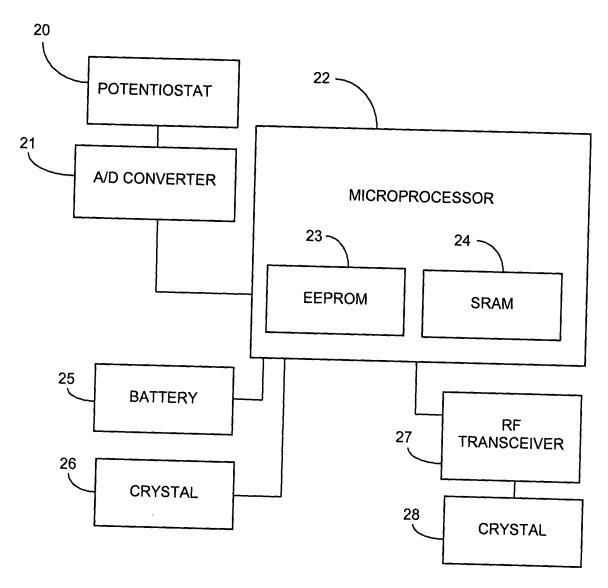


FIG. 2

## SYSTEM AND METHODS FOR PROCESSING ANALYTE SENSOR DATA

Goode, et al.

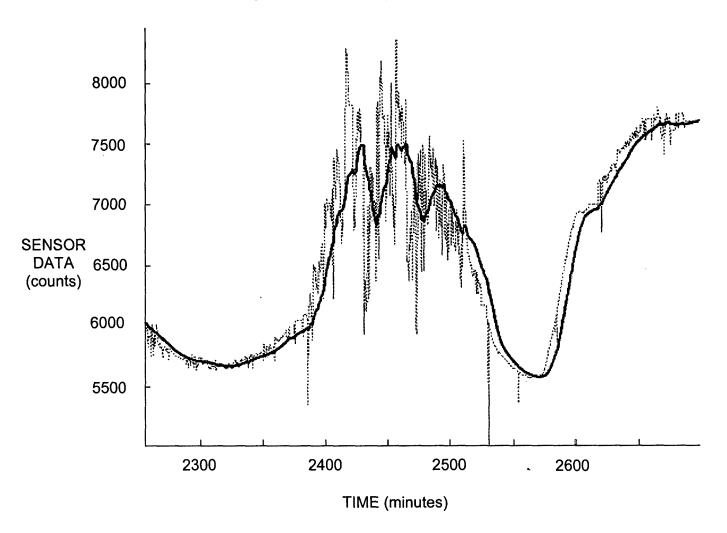


FIG. 3

Appl. No.: Unknown

Atty Docket: DEXCOM.026A

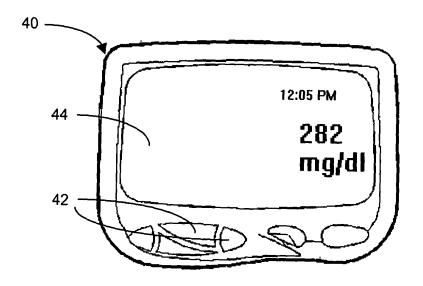


FIG. 4A

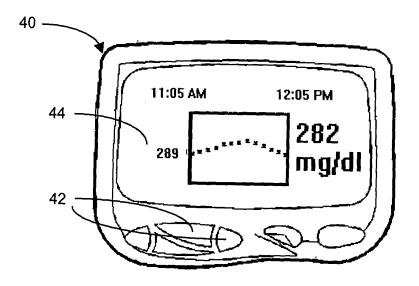


FIG. 4B

Appl. No.: Unknown

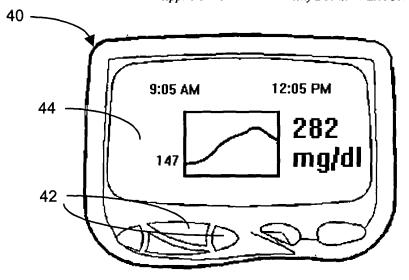


FIG. 4C

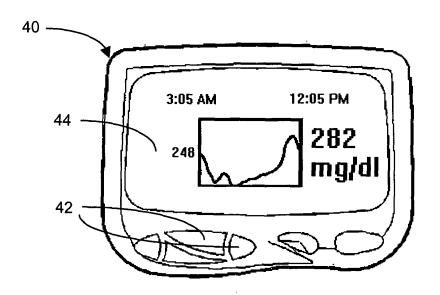


FIG. 4D


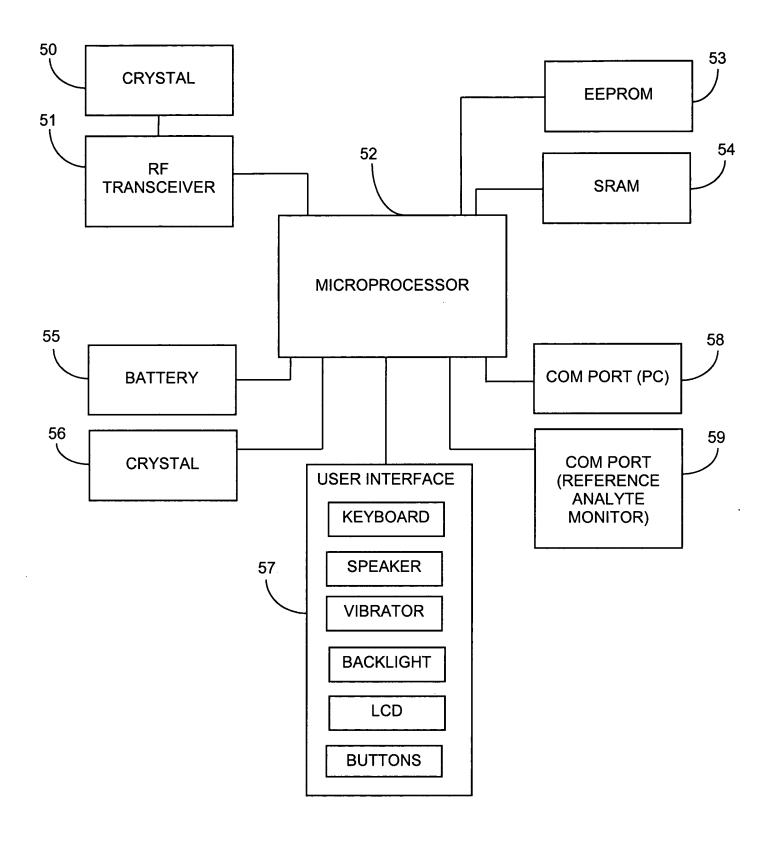



FIG. 5

Appl. No.: Unknown

Atty Docket: DEXCOM.026A

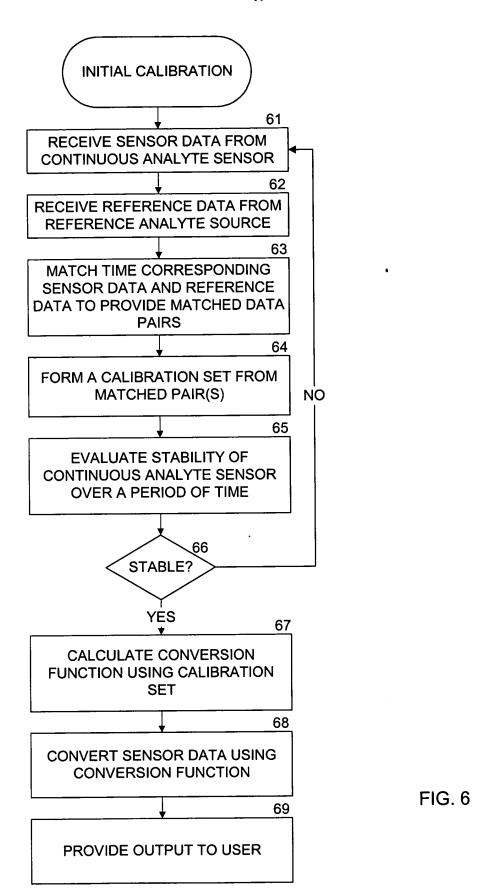

DATA Goode, et al.

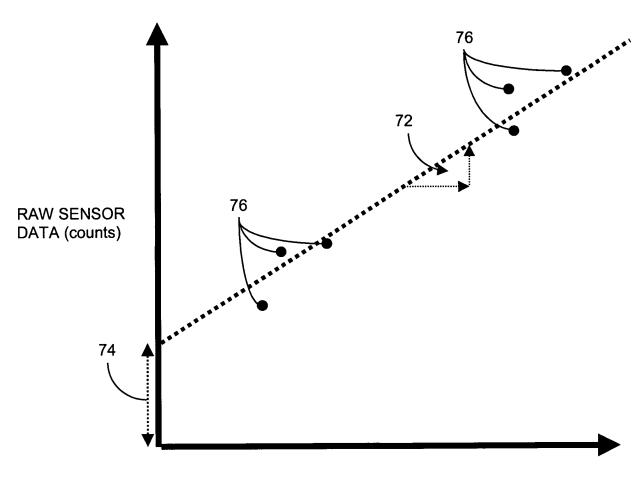

REFERENCE ANALYTE VALUE (mg/dL)

FIG. 7

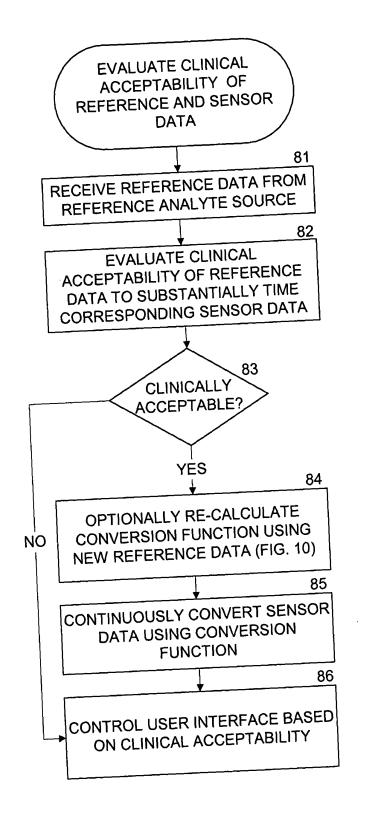


FIG. 8

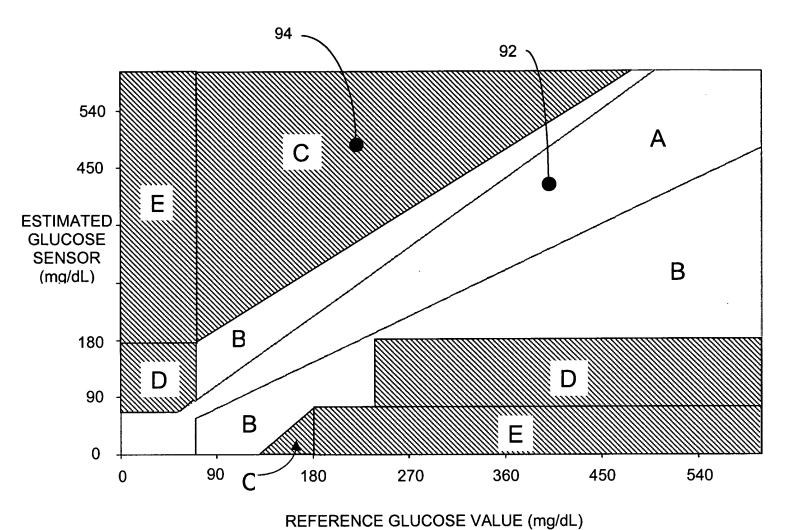


FIG. 9

SYSTEM AND METHODS FOR PROCESSING ANALYTE SENSOR
DATA
Goode, et al.
Appl. No.: Unknown Atty Docket: DEXCOM.026A

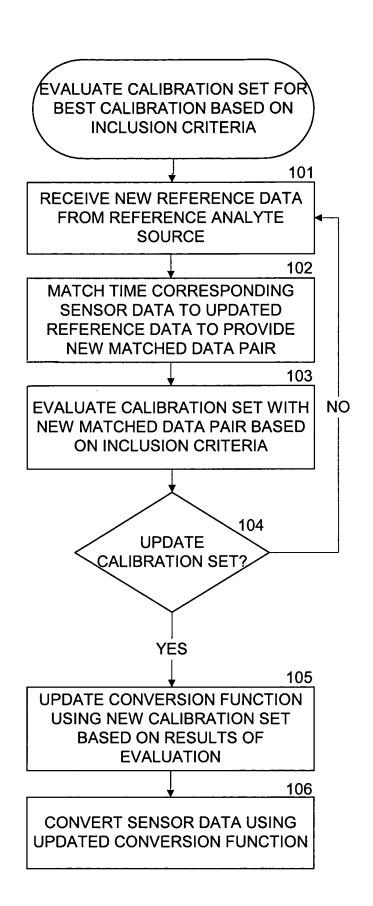


FIG. 10

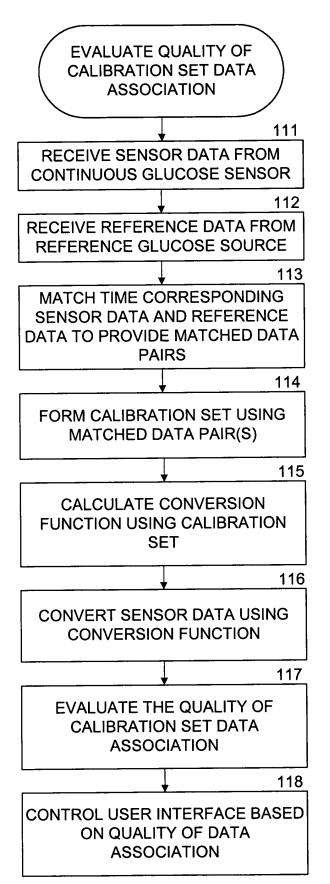


FIG. 11

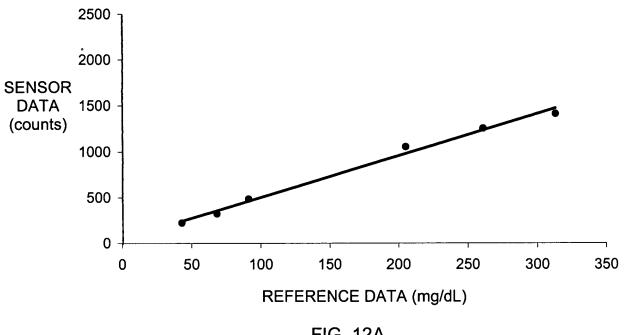


FIG. 12A

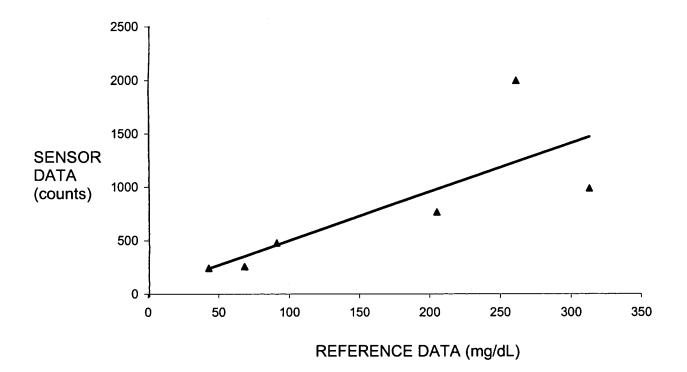


FIG. 12B